

SPECTRA OF PYROELECTRIC X-RAY GENERATOR

V.I. Nagaychenko, V.M. Sanin, A.M. Yegorov, A.V. Shchagin
NSC KIPT, Kharkov 61108, Ukraine

The construction of X-ray generator based on a pyroelectric crystal LiNbO_3 is described. Some properties of radiation spectra from the X-ray generator are presented. Measurements of the spectra were performed at heating and cooling of the crystal with copper and chromium targets. The maximum energy in the X-ray spectrum versus crystal temperature is presented.

PACS: 77.70.+a, 07.85.m

INTRODUCTION

The pyroelectric crystals are known to have an amazing capability for generating electron beams, as their temperature changes [1-8]. The electron beam energy can attain 170 keV [7], depending on the type of crystal, its thickness, heating/cooling conditions. The electric fields generated by pyrocrystals can be as high as 10^6 V/cm [9]. As it has been recently demonstrated, this phenomenon can be used for creating a compact low-power X-ray generator [6,9,10,11]. The basic peculiarities of this generator are the absence of outer high-voltage power source, safety, small size [6,9,10,11]. Here, we present some properties of X-ray spectra from pyroelectric X-ray generator with copper and chromium foils.

1. THE X-RAY GENERATOR

Pyroelectric X-ray generator was created at Kharkov Institute of Physics and Technology. The scheme of the generator is similar to one described in Refs. [6,9,10,11]. It is shown in Fig.1.

The generator uses a pyroelectric crystal LiNbO_3 of size $3.7 \times 4.3 \times 2.5$ mm³, which is subjected to cyclic variations of temperature (heating/cooling) in the temperature range from -50°C to $+120^\circ\text{C}$. The Z – axis of the crystal is along the axis of the generator. A vitrified wire resistor was used for heating, while liquid nitrogen was used for cooling. The cooling line was fabricated from copper rod, and its one end was closely connected with the crystal and the heater, and the other end was immersed in liquid nitrogen. The duration of heating was specified by the resistor current value. The air pressure in the chamber of the generator can be regulated with the help of a variable leak valve and a vacuum pump. The optimum pressure ranges was found between 10 and 50 mTorr. The grounded metal foil serve as a target for generation of X-rays. The spacing between the foil and the crystal surface can be varied from 0 to 15 mm. The X-ray spectra are measured by a semiconductor Si(Li) X-ray detector having a resolution of 250 eV (full width at half height). The brass base and cooling line and target was grounded.

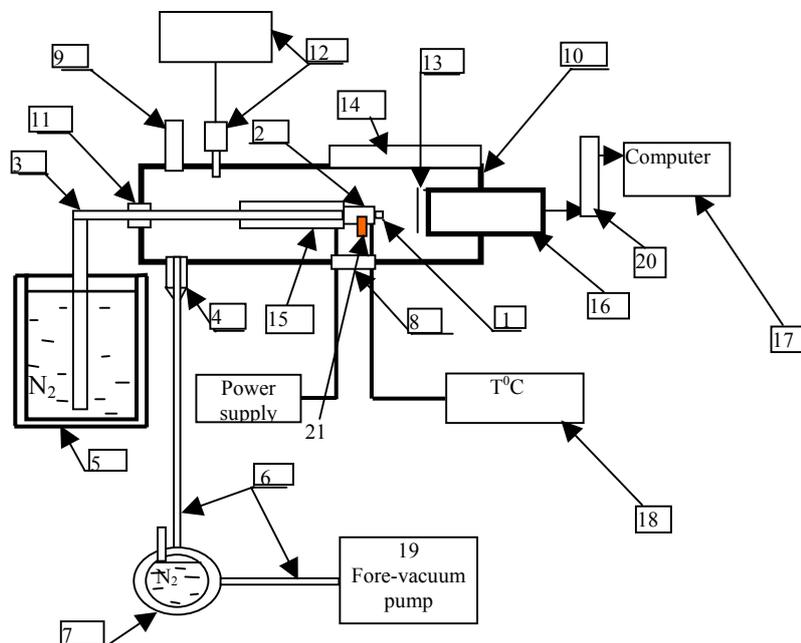


Fig.1. The scheme of the pyroelectric X-ray generator

1 - LiNbO_3 crystal, 2 - brass base, 3 - heating/cooling line, 4 - vacuum valve, 5 - Dewar vessel with liquid nitrogen, 6 - vacuum line, 7 - liquid-nitrogen trap, 8 - vacuum connector, 9 - variable leak valve, 10 - vacuum chamber of the generator, 11 - teflon vacuum obturator of the cooling line, 12 - gas pressure measuring device, 13 - metal foil, 14 - transparent glass window, 15 - resistor-heater, 16 - Si(Li) X-ray detector, 17 - computer, 18 - temperature-measuring device, 19 - fore-vacuum pump, 20 - pulse-height analyzer, 21 - thermocouple

2. X-RAY SPECTRA

The crystal surface on the side of the detector should be charged positively at heating and negatively at cooling. So, at cooling, the electrons can go from the crystal to the target. The target, being bombarded with electrons emits the characteristic X-ray radiation and bremsstrahlung. X-ray radiation spectra measured at cooling with Cu and Cr targets are shown in Figs.2,3 respectively.

At heating, the crystal polarization is reversed and surface, which directed to target, should be charged

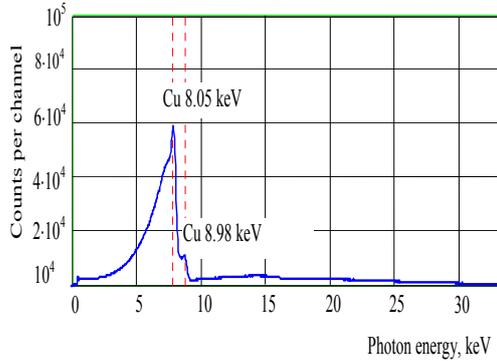


Fig.2. X-ray radiation spectrum measured with Cu target thickness $20 \mu\text{m}$ at LiNbO_3 crystal cooling. The value of one channel is 0.036 keV . The distance between the crystal and the copper foil is 7.5 mm . The total number of counts in the spectrum is $8.391 \cdot 10^6$ for 16 minutes. The residual air pressure in the vacuum chamber is measured to be 25 mTorr

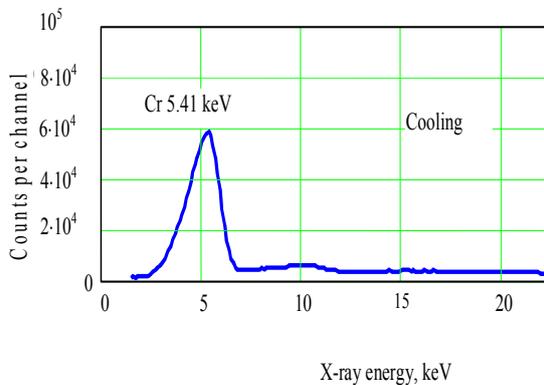


Fig. 3. X-ray radiation spectrum measured with Cr target thickness $18 \mu\text{m}$ at LiNbO_3 crystal cooling for one minute

3. THE MAXIMUM ENERGY OF X-RAYS

Experiments were made to measure the x-ray spectra at dynamic conditions. During a thermal cycle, the several spectra were measured for one minute each.

Eight spectra were measured at LiNbO_3 heating from -50°C up to $+125^\circ\text{C}$. Fig.6 shows a typical dependence of measured maximum energy of X-rays in spectra on the temperature. In this experiment, the crystal of size $3.7 \times 4.3 \times 2.5 \text{ mm}^3$ was used. It is seen from the figure that as the crystal was heated the maximum energy increased up to $\sim 28 \text{ keV}$ (20°C), and

positively. In this case, characteristic X-ray radiation and bremsstrahlung goes from the crystal. This radiation passes through a thin foil and reaches the detector. At crystal heating, the radiation spectra comprises the characteristic K-lines of both crystal and target elements (Figs.4,5). A part of radiation can go from the chamber walls, as the body of the vacuum chamber is made with brass. The registered radiation intensity corresponding to cooling is higher than the one corresponding to heating.

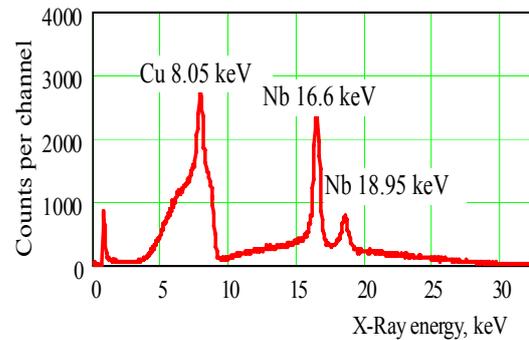


Fig.4. X-ray radiation spectrum measured with Cu foil and crystal elements during LiNbO_3 crystal heating. The distance between the crystal and the copper foil is 7.5 mm . The total number of counts in the spectrum is $4.975 \cdot 10^5$ for 8 minutes. The residual air pressure in the vacuum chamber, which accommodates the crystal, is measured to be 25 mTorr

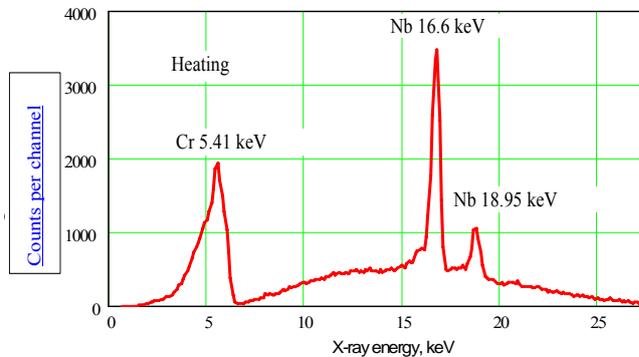


Fig.5. X-ray radiation spectrum measured with Cr target thickness $18 \mu\text{m}$ at LiNbO_3 crystal heating for one minute

then fell off to 17 keV (62°C) with a further rise up to $\sim 30 \text{ keV}$ (120°C). After heating was ceased, the intensity and maximum energy of the x-rays went to zero.

Similar measurements were also conducted on cooling the crystal. A typical curve for the measured maximum energy of radiation versus crystal temperature at cooling conditions is shown in Fig.7. It increases, as the crystal is cooled, and reaches its maximum of $\sim 38 \text{ keV}$ at room temperature ($\sim 20^\circ\text{C}$), then the x-ray maximum energy drops to 0 keV (-40°C).

CONCLUSIONS

The pyroelectric X-ray generator was created in KIPT and its operation was demonstrated. Results of our first experiments are mainly in agreement with the results of earlier pioneer works [6, 8-11].

Continuous part of X-ray spectra in Figs.2-4 should be due to bremsstrahlung of accelerated electrons in a target and crystal. Thus, the maximum energy of X-rays should be close to maximum energy of these electrons.

Therefore, Figs.6,7 show values close to maximum energy of electrons in the generator.

ACKNOWLEDGMENTS

We are thankful to S.M. Shafroth and J.D. Brownridge for encourage to start works in this field and J.D. Brownridge for gift of pyrocrystals for our first experiments, and to Crystal Technology Inc. what supplied us with pyrocrystal samples. The work was performed on STCU 1911 project.

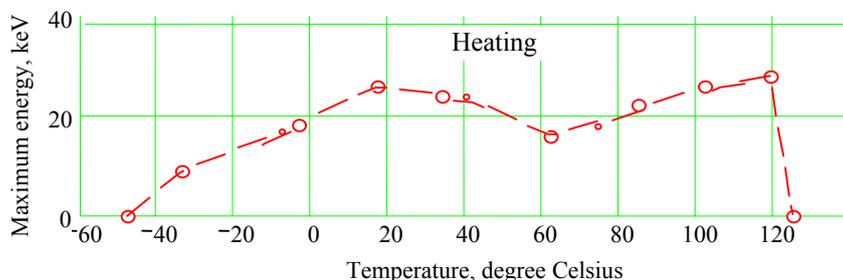


Fig. 6. Maximum energy of X-rays versus crystal temperature at heating conditions

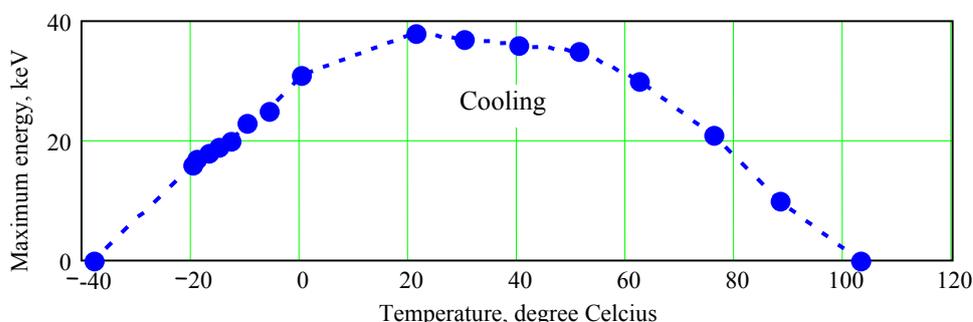


Fig.7. Maximum energy of X-rays versus crystal temperature at cooling conditions

REFERENCES

1. B. Rosenblum, P. Brunlich and J.P. Carrico. // *Appl. Phys. Lett.* **25**, 17(1974).
2. I.V. Strigushenko, S.G. Dmitriev and O.V. Silant'eva // *Sov. Phys. J Solid State* **19**, 1171 (1977).
3. V.S. Kortov, K.K. Shvarts, A.F. Zatsepin, A.I. Gaprindashvili, A.V. Gulbis and Z.A. Grant // *Sov. Phys. J Solid State* **21**, 1092 (1979).
4. V.S. Kortov, A.F. Zatsepin, A.I. Gaprindashvili, M.M. Pinaeva, V.S. Vasil'ev and I.A. Morozov // *Sov. Phys. Tech. Phys.* **25**(9) 1126 (1981).
5. J. Kalinovski and Z. Ddreger // *Phys.Rev.* **B 36**, 7840 (1987).
6. J.D. Brownridge, S.M. Shafroth, D. Trott, B. Stoner, W. Hooke // *Appl. Phys. Lett.* **78**, 1158 (2001).
7. G. Rosenman, D. Shur, Ya.E. Krasik, and A. Dunaevsky // *J. Appl. Phys.* **88**, 6109 (2000).
8. J.D. Brownridge, S.M. Shafroth: Electron preprint <http://arxiv.org/pdf/physics/0209079>
9. J.D. Brownridge, *Nature*, **358**, 287-288 (1992).
10. James Brownridge and Sol Raboy // *J. Appl. Phys.* **86**, 640 (1999).
11. S.M. Shafroth, W. Kruger and J.D. Brownridge. Time dependence of X-ray yield for two crystal X-ray generators // *Nucl. Instr. and Meth.*, **A 422**, 1-4 (1999).

СПЕКТРЫ ОТ ПИРОЭЛЕКТРИЧЕСКОГО РЕНТГЕНОВСКОГО ГЕНЕРАТОРА

В.И.Нагайченко, В.М.Санін, А.М.Егоров, А.В.Щагин

Описана конструкция рентгеновского генератора, основанного на пироэлектрическом кристалле LiNbO_3 . Представлены некоторые свойства спектров излучения от рентгеновского генератора. Измерения спектров были выполнены при нагревании и охлаждении кристалла с мишенями из меди и хрома. Представлена максимальная энергия рентгеновского спектра в зависимости от температуры кристалла.

СПЕКТРИ ВІД ПІРОЕЛЕКТРИЧНОГО РЕНТГЕНІВСЬКОГО ГЕНЕРАТОРА

В.І.Нагайченко, В.М.Санін, О.М.Егоров, А.В.Щагін

Описано конструкцію рентгенівського генератора, заснованого на піроелектричному кристалі LiNbO_3 . Наведені деякі властивості спектрів випромінювання від рентгенівського генератора. Виміри

спектрів були виконані при нагріванні й охолодженні кристалу з мішенями з міді і хрому. Представлено максимальну енергію рентгенівського спектру в залежності від температури кристалу.